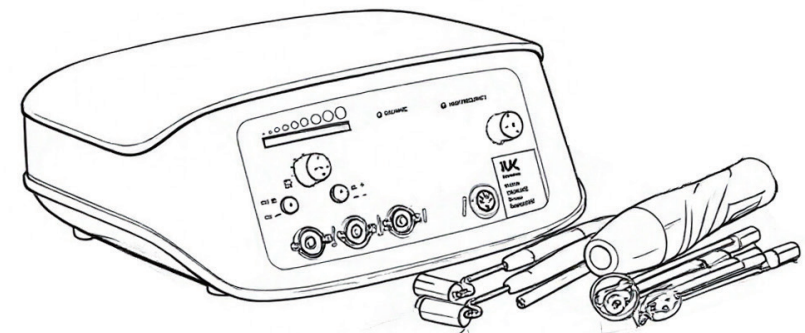


Instructions Manual

Beauty instrument

F803.N

GALVANIC & HIGH FREQUENCY



WK
Imported by
WEELKO BARCELONA SL

Pol. Ind. La Vall d'an
Camí de Garreta, 92
08600 Berga
Barcelona - Spain
T. +34 93 824 90 20
E. info@weelko.com

VERSION 1.0

Thank you sincerely for choosing our product. This manual is compiled to help users operate this instrument effectively. We hope our company's products and services will bring you a distinguished experience.

This user manual contains all general information about the instrument. It serves as the starting point for new users to begin using the instrument, as it provides a general introduction to the system, explains how it works, and details the instrument's installation and various operation methods.

Usage Precautions

1. Before turning on the machine, be sure to read the user manual carefully. Operators must be familiar with the user manual and operation methods, and the instrument must be managed by a designated person;
2. Do not use a power strip to avoid fire hazards;
3. When replacing the fuse, always turn off the power switch to prevent fire and electric shock;
4. Must use a power supply of $220V\pm 22V$, $50HZ\pm 1HZ$ and an effectively grounded socket;
5. Using a damaged or modified power cord may cause fire and electric shock hazards;
6. If the instrument is loose, falling, or damaged, please contact the company in a timely manner;
7. Do not use the instrument in unstable environments such as tilting, vibrating, or impacting conditions;
8. No water or debris is allowed to enter the interior of the instrument. In case of foreign objects entering, please contact the company promptly;
9. When moving the instrument, the power plug must be pulled out first;
10. When moving the instrument, try to avoid vibration;
11. The instrument should be placed on a stable surface, with at least 5cm of space left around it to ensure air circulation and facilitate heat dissipation of the instrument;
12. Do not cover the instrument with anything to prevent blockage of the air vents;
13. Avoid using the instrument in the following environments: direct sunlight; high humidity environments; near water; vibrating or tilting places; strong magnetic field environments; places where electromagnetic waves or impulse voltages occur; places where chemicals are stored or corrosive gases exist;

Product Packaging List

Name	Image Quantity
Main Unit	1
Galvanic Roller Handles	2
Galvanic Handheld Stick	1
High-Frequency Handle	1
Tongue-Shaped Electrotherapy Tube	1
Straight Electrotherapy Tube	1
Curved Electrotherapy Tube	1
Mushroom-Shaped Electrotherapy Tube	1
Power Cord	1

Product Packaging List

- Input Voltage: AC 220V-240V
- Product Frequency: 50/60HZ
- Product Power: 15W
- Packaging Dimensions: 34x34x22CM
- Gross Weight: 3.2KG
- Net Weight: 2.8KG

14. This instrument shall not be placed or used near radios, televisions, copiers, fax machines, etc.;
15. Do not use it together with other instruments (such as microwaves) to avoid mutual interference between instruments and cause misoperation;
16. If an abnormal situation occurs to the instrument or the user during operation, the operator shall immediately move the operation handle away from the user, press the stop switch, and stop using the instrument;
17. The instrument shall be correctly used by skilled operators. Personnel other than operators are not allowed to use the instrument;
18. After the operation, place the control handle back on the control handle holder;
19. After using the operation handle, clean the probe thoroughly for next use.

Precautions for Troubleshooting, Storage, and Inspection

1. Do not use the instrument if it malfunctions. In case of smoke, burning smell, or inability to operate, continued use may cause fire or electric shock. Immediately press the stop button, turn off the power, unplug the power plug, and contact the company or distributor immediately;
2. Personnel other than professional technicians are strictly prohibited from repairing or modifying the instrument. The interior of the instrument must never be opened;
3. The instrument and its components must be inspected regularly;
4. Do not use cleaning tools that may damage the instrument's protective coating, such as brushes, brooms, etc.;
5. If the instrument is not used for more than 2 weeks, it must be carefully inspected before reuse.

Contraindicated Groups

(Do Not Use If You Belong to the Following Groups)

1. Individuals with implanted cardiac pacemakers, defibrillators, or metal implants (such as steel plates, bone nails) in the body;
2. Pregnant women, lactating women, and women during menstruation;
3. Patients with epilepsy, hypertension, severe heart disease, diabetes, tumors or cancer, or thyroid diseases;
4. Individuals with open wounds, skin damage, severe inflammation, eczema, dermatitis on the skin, or those with facial telangiectasia (spider veins) or rosacea;
5. Those who have received botulinum toxin injections, filler injections, laser treatments, chemical peels, or plastic surgery recently (usually within 6 months).

Operation Process

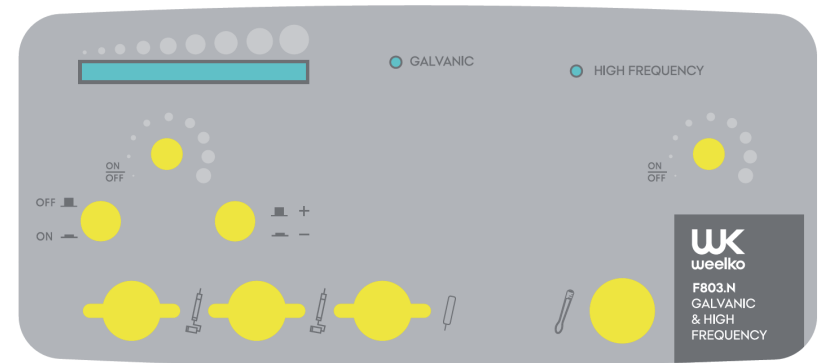
1. Pre-Use Preparation

- Inspect the Instrument: Ensure the instrument is dry and intact, and the glass electrotherapy tube is clean and free of cracks;
- Prepare the Skin: Thoroughly clean the face to ensure the treatment area is dry and free of cosmetics or oil;
- Connect the Electrode: First select and insert the appropriate glass electrotherapy tube, then turn on the power;
- Apply Medium: Apply a sufficient amount of special conductive gel or essence on the skin. Dry operation is strictly prohibited to provide conductivity and avoid burns.






2. Post-Use Operation

- Shutdown Sequence: First adjust the intensity knob back to the lowest gear or "0" position, then turn off the power;
- Remove the Electrode: After turning off and unplugging the power, carefully remove the glass electrotherapy tube. Do not pull it hard;
- Cleaning and Maintenance: Clean the instrument handle and electrotherapy tube with a soft damp cloth, and store them in a cool and dry place after drying.

Instrument Operation Steps



Instrument Operation Steps

1. Connect the device to a 220V power supply. The device will emit a "beep" sound, indicating that it is powered on and enters standby mode;
2. Insert the Galvanic accessory handles according to the marks . Insert the high-frequency handle according to the accessory mark , and insert the selected electrotherapy tube before use;
3. Use the  switch to turn on/off the Galvanic function;
4. Press the  button to switch between Galvanic Import/Export modes;
5. Adjust the Galvanic energy from low to high using the knob. There are 10 energy levels with corresponding indicator lights;
6. Use the  (HIGH FREQUENCY) switch to turn on/off the high-frequency function, and adjust the energy from low to high;
7. After setting, start the corresponding function for treatment. Follow the operation techniques and duration requirements in the respective function sections;
8. After the operation, turn off the power, remove the handles and electrotherapy tubes, clean them thoroughly, and store the instrument in a dry and cool place.